LABORATORY

AL-TR-1991-0011

AD-A260 579





THE EFFECT OF SIGNAL-TO-NOISE RATIO ON VISUAL ACUITY THROUGH NIGHT VISION GOGGLES

Joseph T. Riegler

LOGICON TECHNICAL SERVICES, INC. DAYTON, OH 45431-7258

> James D. Whiteley, Ph.D. H. Lee Task, Ph.D. James Schueren, M.S.

CREW SYSTEMS DIRECTORATE HUMAN ENGINEERING DIVISION

93-03866

MARCH 1991



INTERIM REPORT FOR PERIOD OCTOBER 1989 TO SEPTEMBER 1990

Approved for public release; distribution is unlimited.

98

AIR FORCE SYSTEMS COMMAND WRIGHT-PATTERSON AIR FORCE BASE, OHIO 45433-6573

NOTICES

When US Government drawings, specifications, or other data are used for any purpose other than a definitely related Government procurement operation, the Government thereby incurs no responsibility nor any obligation whatsoever, and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise, as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

Please do not request copies of this report from the Armstrong Aerospace Medical Research Laboratory. Additional copies may be purchased from:

National Technical Information Service 5285 Royal Road Springfield, Virginia 22161

Federal Government agencies and their contractors registered with the Defense Technical Information Center should direct requests for copies of this report to:

Defense Technical Information Center Cameron Station Alexandria, Virginia 22314

TECHNICAL REVIEW AND APPROVAL

AL-TR-1991-0011

This report has been reviewed by the Office of Public Affairs (PA) and is releasable to the National Technical Information Service (NTIS). At NTIS, it will be available to the general public, including foreign nations.

The voluntary informed consent of the subjects used in this research was obtained as required by Air Force Regulation 169-3.

This technical report has been reviewed and is approved for publication.

FOR THE COMMANDER

Gennett R Soff

KENNETH R. BOFF

Acting Division Chief

Human Engineering Division

Armstrong Laboratory

REPORT DOCUMENTATION PAGE

Form Approved OMB No 0/04 0188

1. AGENCY USE ONLY (Leave blank)	2. REPORT DATE February 1991	Final, Oct 89 to Sep 90
. TITLE AND SUBTITLE	<u> </u>	5. FUNDING NUMBERS
The Effect of Signal-to-	Voise Ratio on Vis	aal PE 62202F
cuity Through Night Vis	ion Goggles (U)	PR 7184 TA 18
AUTHOR(S)		WU 07
Riegler, Joseph T.		C F33615-89-C-0532
Whiteley, James D., Capt		
Task, H. Lee, PhD; Schuo		pt, USAF
PERFORMING ORGANIZATION NAME	• • • • • • • • • • • • • • • • • • • •	8. PERFORMING ORGANIZATION REPORT NUMBER
Logicon Technical Servic	res, Inc.	Rev OAT Admite
P.O. Box 317258		
Dayton OH 45431-7258		·
SPONSORING MONITORING AGENCY	NAME(S) AND ADDRESSIE	5) 10 SPONSORING MONITORING
Armstrong Laborator		AGENCY REPORT NUMBER
Crew Systems Direct		AL-TR-1991-0011
Human Engineering D		
AFSC, HSD		
Wright-Patterson AF	L, OH 45433-657	3
Ra. DISTRIBUTION AVAILABILITY STAT	EMENT	126 DISTRIBUTION CODE
Approved for public relea	ise;	1
istribution is unlimited	l. ·	A
A0(10.67 a)	22	vision goggles (NVGs) have been used by
environment. The key concurrently, no studies were of image intensitiers to was to determine the effective, using PVS-7 third quarter moon and starlight Hifferent SNRs. The rangussessed using Landolt of Histance at which the according intensitier tube SNR to visual acuity for develop predictive guide	ersonnel to perform ponent of these does identified which human visual acrification NVGs, at illumination lease of SNR examined charts with target strast conditions. The illumination of the session were performed each experimental line tables to pro-	wisual operations in a nightfine evices is the image intensifier tube. In relate the signal-to-noise ratio (SNR) two. The purpose of the present research fier tube sNR on visual acuity. Visual was measured for twelve participants at wells for four intensifier tubes with was 11.0% to 17.0%. Visual acuity was tocontrasts of 20 to 95 percent. The resolved was recorded for each of the line results showed that increases in evel, and contrast affected visual doubtain estimated equations relating condition. The results were used to wide approximate percent degradation/ atensitier tube signal-to-noise ratio.
1. SUBJECT TERMS		15 NUMBER OF PAGES
		25
•	Night Vision Oggi	16 PRICE CODE
	Image intensifier	

SECURITY CLASSIFICATION OF ABSTRACT

SECURITY CLASSIFICATION OF THIS PAGE

UNCLASSIFIED

II.

20 LIMITATION OF ABSTRACT

OF REPORT

SECURITY CLASSIFICATION

GENERAL INSTRUCTIONS FOR COMPLETING SF 298

The Report Documentation Page (RDP) is used in announcing and cataloging reports. It is important that this information be consistent with the rest of the report, particularly the cover and title page instructions for filling in each block of the form follow. It is important to stay within the lines to meet optical scanning requirements.

- Block 1 Agency Use Only (Leave blank)
- **Block 2.** Report Date Full publication date including day, month, and year, if available (e.g. 1 Jan 88). Must cite at least the year
- Block 3. Type of Report and Dates Covered State whether report is interim, final, etc. If applicable, enter inclusive report dates (e.g. 10 Jun 87 30 Jun 88).
- Block 4. <u>Title and Subtitle</u> A title is taken from the part of the report that provides the most meaningful and complete information. When a report is prepared in more than one volume, repeat the primary title, add volume number, and include subtitle for the specific volume. On classified documents enter the title classification in parentheses.
- Block 5. Funding Numbers To include contract and grant numbers; may include program element number(s), project number(s), task number(s), and work unit number(s). Use the following labels.

C Contract PR Project
G Grant TA Task
PE Program WU Work Unit
Element Accession No

- Block 6. Author(s) Name(s) of person(s) responsible for writing the report, performing the research, or credited with the content of the report. If editor or compiler, this should follow the name(s)
- Block 7. <u>Performing Organization Name(s)</u> and <u>Address(es)</u> Self-explanatory
- Block 8. <u>Performing Organization Report</u>
 <u>Number</u> Enter the unique alphanumeric report number(s) assigned by the organization performing the report
- **Block 9.** Sponsoring/Monitoring Agency Name(s) and Address(es) Self-explanatory
- **Block 10**. Sponsoring/Monitoring Agency Report Number (If known)

Block 11. Supplementary Notes Enter information not included elsewhere such as Prepared in cooperation with . Trans of . To be published in ... When a report is revised, include a statement whether the new report supersedes or supplements the older report.

Block 12a. <u>Distribution/Availability Statement.</u> Denotes public availability or limitations. Cite any availability to the public. Enter additional limitations or special markings in all capitals (e.g. NOFORN, REL, ITAR) おかけいのはないとはなるとなるとなるとなるとなっているとうないとうないとうと

DOD See DODD 5230 24, "Distribution

Statements on Technical

Documents "

DOE See authorities

NASA See Handbook NHB 2200 2

NTIS - Leave blank

Block 12b. Distribution Code

DOD - Leave blank

 DOE - Enter DOE distribution categories from the Standard Distribution for Unclassified Scientific and Technical Reports

NASA - Leave blank NTIS - Leave blank

- Block 13. Abstract Include a brief (Maximum 200 words) factual summary of the most significant information contained in the report
- **Block 14.** <u>Subject Terms</u> Keywords or phrases identifying major subjects in the report
- **Block 15**. Number of Pages. Enter the total number of pages.
- **Block 16** Price Code Enter appropriate price code (NTIS only)
- Blocks 17. 19. Security Classifications Selfexplanatory Enter U.S. Security Classification in accordance with U.S. Security Regulations (i.e., UNCLASSIFIED). If form contains classified information, stamp classification on the top and bottom of the page.
- Block 20. <u>Limitation of Abstract</u> This block must be completed to assign a limitation to the abstract. Enter either UL (unlimited) or SAR (same as report). An entry in this block is necessary if the abstract is to be limited. If blank, the abstract is assumed to be unlimited.

Summary

The purpose of the present research was to determine the effect of NVG image intensifier tube signal-to-noise ratio (SNR) on visual acuity. Visual acuity through PVS-7 NVGs was measured for twelve subjects at quarter moon and starlight illumination levels for four intensifier tubes with different SNRs. The range of SNRs examined was 11.37 to 17.92. Visual acuity was assessed using Landolt C charts with target contrasts of 20 and 95 percent. The results showed that image intensifier tube SNR, illumination level, and contrast had significant effects on visual acuity. Regression analyses were performed to obtain estimated equations relating SNR to visual acuity for each illumination and contrast condition.

The results showed a trend toward SNR having a greater impact on visual acuity at the two lowest illumination conditions than at the higher illumination condition. The results were used to produce guideline tables for estimating percent increases in visual acuity as a function of intensifier tube SNR. Due to the large differences between subjects in visual acuity performance with NVGs, it was concluded that further research should be conducted to examine the correlation between visual acuity obtained for unaided normal room light viewing and NVG viewing.

DITO QUALITY LIMIT OF THE 3

ngio kalai Dalo bis Na angan		
·		
	,	-
D 1	;	

Preface

This evaluation was completed under work unit 7184-18-07 by members of the Crew Systems Effectiveness Branch, Human Engineering Division, Armstrong Acrospace Medical Research Laboratory, Wright-Patterson Air Force Base, Ohio and Logicon Technical Services, Inc., Dayton, Ohio. The authors thank Annette Zobel (LTSI) for her technical support throughout this study and Chuck Goodyear (LTSI) for his assistance with data analysis and interpretation.

Contents

1	Intr	roduction	1											
2	Met	ethod												
	2.1	Subjects	;											
	2.2	Facilities and Equipment	:											
	2.3	Stimuli	į											
	2.4	Procedure	•											
	2.5	Experimental Design	8											
3	Res	ults	9											
	3.1	ANOVA Results	ć											
	3.2	Regression Analysis	1											
4	Dis	cussion	15											
5	Apı	pendix	2											

List of Figures

2.1	AAMRL Zoom Lane Laboratory	4
2.2	Change in Landolt C gap angular subtense as a function of zoomlane distance	
	for 20% and 95% letters	6
3.1	Mean visual acuity as a function of SNR, illumination, and contrast	10
3.2	Mean visual acuity as a function of tube SNR and illumination averaged	
	across contrast	10
3.3	Mean visual acuity as a function of illumination and contrast averaged across	
	SNR	11
3.4	Plots of estimated equations depicting relationship between SNR and visual	
	acuity for each illumination and contrast condition	13

List of Tables

2.1	Moon illumination and acuity chart luminance values used in present exper-	
	iment	7
3.1	Estimated Equations for each illumination and contrast condition	14
3.2	Percent increase in visual acuity from a lower SNR (left column) to a greater	
	SNR (top row) between the SNRs used in this study	14
3.3	Estimated equations with tube SNR 15.28 excluded from analysis	14
4.1	Prediction Matrix for SNR-Visual Acuity .01 Moon 20% Contrast	17
4.2	Prediction Matrix for SNR-Visual Acuity .01 Moon 95% Contrast	17
4.3	Prediction Matrix for SNR-Visual Acuity .25 Moon 20% Contrast	18
4.4	Prediction Matrix for SNR-Visual Acuity .25 Moon 95% Contrast	18
5.1	Analysis of Valiance (ANOVA) Summary Table	21

Introduction

Night vision goggles (NVGs) have been developed by the US Army for use in night military operations. The key component of these devices is the image intensifier tube. The image intensifier tube is basically a light amplifier that is sensitive over the spectral region of about 600nm to 900nm (for the third generation intensifier). There are a number of parameters that are used to characterize the image intensifier such as gain, resolution, brightness, distortion, signal-to-noise ratio, etc (see Csorba [1]). Measurement procedures exist for determining the value of these parameters and others. However, there have been very few studies that relate these parameters to their impact on human visual performance with the NVGs. Specifically, no studies could be found that related the signal-to-noise ratio (SNR) with human visual acuity even though there exist specifications as to the SNR required for image intensifiers.

The purpose of the study described herein was to determine the effect of SNR on visual acuity. Four TVS-7, third generation image intensifier tubes were acquired that had four different SNRs. The PVS-7 tube was chosen because the PVS-7 NVGs use a single objective lens and a single image intensifier that is imaged to both eyes via beamsplitting optics and two eyepieces. This allowed the subject to observe the image through the NVGs with both eyes.

Visual acuity is normally measured by determining the minimum angular subtense of a specified test character (e.g. Landolt "C", tumbling "E", or Snellen letter) at which an observer can determine the orientation of the character (Landolt "C", tumbling "E") or be able to read the character (Snellen letters). A typical eye chart used for this type of measurement consists of lines of characters of different sizes. However, these charts are designed for use in vision screening and, due to the character size increments, are not very well suited for research.

Two other factors that affect visual acuity (both direct view and through night vision goggles) are contrast and illumination level. Visual acuity tends to be poorer for

lower contrast levels and lower illumination levels.

Based on this information, it was decided to investigate visual acuity with the PVS 7 NVGs for two different illumination levels and two different contrasts. It was also necessary to develop a methodology by which the angular subtense of the visual acuity test character could be made continuously variable to permit more accurate determination of acuity. Since angular subtense depends on the distance from the subject to the test target, a technique was used that continuously varied this distance in a controlled fashion. The subject was seated in a cart that moved at a uniform speed along a track toward the test target. This methodology provided an excellent means of getting a sensitive measure of visual acuity.

Method

2.1 Subjects

Twelve male volunteers participated in this study. The subjects ranged in age from 18 to 34 years (mean = 23.8, SD = 5.0). Each subject reported good ocular health and visual acuity of at least 20/20 corrected in each eye for distance vision.

2.2 Facilities and Equipment

The facility used for data collection was the zoom lane, see Figure 2.1, located in the Visual Dynamics Facility, Armstrong Aerospace Medical Research Laboratory, Human Engineering Division, Wright-Patterson AFB, Ohio. The equipment comprising the zoom lane was an electronically controlled cart powered by an electric motor and operated via a retractable cable system. The cart itself contained a height adjustable, high-backed seat, a side stick controller to input cart stop commands and an armrest to reduce arm fatigue during the experiment. A black plexiglass board was positioned on the front of the cart such that it could be raised to occlude vision between experimental runs. The subject was seated inside the cart, which traveled along a 12.2 meter (m) track. System control was provided by a Zenith 248 computer, which allowed the experimenter to input movement commands (e.g., starting, stopping, velocity and direction) and data collection functions from a remote control panel.

A moonlight simulator was used to approximate the spectral characteristics and luminance intensity levels of different phases of the moon. It was mounted on a tripod which was adjusted to provide calibrated illumination on the surface of the Landolt C charts used as visual stimuli for assessing visual acuity. A Photo Research PR-1980b Pritchard Photometer was used to measure the photometric luminance of the charts and background. This was performed several times during each session to verify that the luminance of the

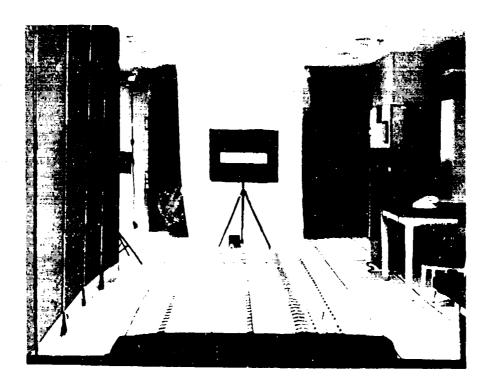


Figure 2.1: AAMRL Zoom Lane Laboratory

chart remained constant.

A pair of ITT AN/PVS-7B biocular night vision goggles (NVGs) were used as the optical test platform for this research. Four ITT third generation image intensifier tubes with similar characteristics, but different signal-to-noise ratios were used.

The AN/PVS-7B NVGs, like most NVGs, have a relatively fast (low Finumber) objective lens to gather as much light as possible to enhance performance of the NVGs. However, this low Finumber also reduces the depth of focus of the NVGs which, for the present experimental procedure, posed a problem. Since the dependent variable of this experiment was the angular subtense of the acuity target obtained by varying the distance from the observer to the chart, a large depth of focus was required. The depth of focus needed to be sufficiently large that the quality of the image would not be degraded over the zoom lane cart distance range (12.2 to 3.05 m; see Fig 2.2).

Depth of focus can easily be increased by reducing the objective lens aperture of the NVGs. However, this reduces the irradiance produced by the lens at the input side of the image intensifier tube. This effect can be corrected by increasing the radiance of the target

to compensate for the light energy lost due to reducing the objective lens aperture. Since the irradiance at the image plane of a lens (the input side of the NVGs in this case) is proportional to the square of the clear aperture of the lens (usually the lens diameter), then the revised radiance necessary can be calculated from the square of the ratio of the original lens diameter to the modified lens system diameter (the aperture placed over the lens). The PVS-7 lens has an effective diameter of 20.8 mm. and the aperture used to increase depth of focus was 4 mm. Thus the target radiance was increased by a factor of $(\frac{20.8}{1})^2$ or 27. Table 2.1 lists some converted values used for this study.

2.3 Stimuli

Visual Acuity Charts

The Landolt C chart format was chosen as the visual stimulus for measuring acuity in this study. Visual acuity was assessed for two levels of positive letter-to-background contrast, 20 and 95 percent. Modulation contrast (C) was calculated using the following equation:

$$C = \frac{Backgrnd_{Lum} - Target_{Lum}}{Backgrnd_{Lum} + Target_{Lum}}$$

A visual acuity of 20/20 represents detection of a gap width (open end of C) subtending 1 minute of arc, using the Landolt C procedure. The Landolt C letter size is five times its gap width. Two letter sizes were used to ensure that both the high and low contrast letters would remain in focus and could be resolved within the zoomlane range (12.2 m to 3.05 m). Letters having gap widths of 4.7 mm and 7.6 mm were used for the high and low contrast conditions, respectively. These represented Snellen fraction sizes of 20/36 and 20/57 at a distance of 9.1 m (30 ft.). The Landolt Cs were displayed on acuity charts which measured 0.15 m by 0.61 m and contained high contrast or low contrast letters on a white background. The letters were separated by a distance of 70 mm.

Each trial was initiated at a distance of 12.2 m from the acuity chart. The trial ended when the subject was able to determine the orientation of each C on the chart. The change in angular subtense of the Landolt C gap as a function of distance from the acuity chart is plotted in Figure 2.2 for both high and low contrast letters.

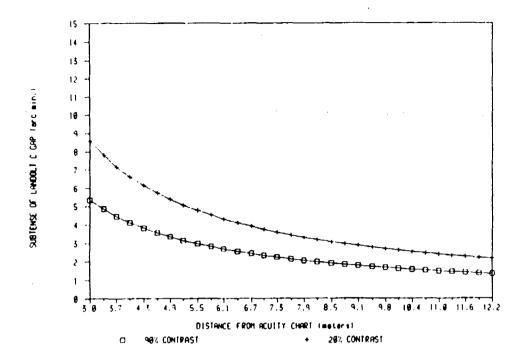


Figure 2.2: Change in Landolt C gap angular subtense as a function of zoomlane distance for 20% and 95% letters

Luminance Levels

The Landolt C target stimuli were presented on white foam core boards having a reflectance of approximately 100 percent. Since there is a convention in the night vision goggle community to relate illumination levels to fraction of moon illumination, it was necessary to make some assumptions in order to arrive at an appropriate reflected luminance level from the target test chart.

The first concern was determining what level of illumination was considered to be "full moon". From the RCA Electro-Optics Handbook [2], a value of 0.0235 foot-Candles (ft.-C) illumination is listed as maximum full moon illumination. It should be noted that actual moon illumination depends heavily on weather conditions (light haze can reduce illumination considerably), moon elevation level above the horizon, and orientation of the surface illuminated. Further, the vast majority of naturally occurring objects ave a reflectance factor considerably less than unity, thus reducing the apparent luminance of the object. For purposes of this study, it was decided to have the white areas of the stimulus target simulate a 50% reflective Lambertian (fully scattering) surface. Due to the way English units of luminance and illuminance are defined, one foot-candle of illumination gives rise to one foot-Lambert of luminance for illumination falling on a perfect Lambertian reflector with unity reflectance.

Table 2.1: Moon illumination and a uity chart luminance values used in present experiment

MOON	DESIRED	ASSUMED	DESIRED	ADJUST.	REQ. CHART
ILLUM.	ILLUM.	REFLECT.	LUM.	FACTOR	LUMINANCE
LEVEL	(FtC)	(percent)	(FtL)		(FtL)
Full	0.0235	50	0.0118	27	0.3186
0.25	0.00588	50	0.00294	27	0.0794
0.01	0.000235	50	0.000118	27	0.0032
	ILLUM. LEVEL Full 0.25	ILLUM. ILLUM. LEVEL (FtC) Full 0.0235 0.25 0.00588	ILLUM. ILLUM. REFLECT. LEVEL (FtC) (percent) Full 0.0235 50 0.25 0.00588 50	ILLUM. ILLUM. REFLECT. LUM. LEVEL (FtC) (percent) (FtL) Full 0.0235 50 0.0118 0.25 0.00588 50 0.00294	ILLUM. ILLUM. REFLECT. LUM. FACTOR LEVEL (FtC) (percent) (FtL) Full 0.0235 50 0.0118 27 0.25 0.00588 50 0.00294 27

Based on these assumptions: 1) full moon illumination is 0.0235 ft.-C, 2) the stimulus target is Lambertian (perfectly diffusing); and 3) a 50% reflective surface is desired, the simulated moon illumination source should, for full moon illumination, be adjusted to provide an illumination of 0.0235/2 or 0.0118 ft.-C, which gives rise to 0.0118 ft.-L luminance, at the white areas of the target. This value is for the NVGs with no aperture over the lens. If the aperture is in place, this value needs to be increased by a factor of 27 as discussed earlier. Table 2.1 lists the fractional moon illumination levels, the corresponding target luminance that would result from a 50% reflective surface, and the luminance that was required to compensate for the 4mm aperture over the objective lens of the NVGs.

2.4 Procedure

Training Trials

Prior to data collection each subject participated in one block of eight trials; two at each illumination and contrast condition. These trials served to familiarize subjects with the task while allowing for dark adaptation. Each subject was individually tested following the same procedure outlined for the data collection trials. On each training trial, subjects were presented a chart containing four Landolt Cs of diminishing size. Subjects stopped the cart and called out the orientation of each C in succession, starting with the largest. The cart was advanced forward until each C orientation was correctly identified.

Data Collection Trials

Each subject performed the experiment seated in the cart which moved at a constant velocity of 0.25 meters per second toward the acuity chart. At the beginning of each trial,

the cart was positioned so that the subject's eyes were at a distance of 12.2 m from the acuity chart. During data collection, all the Landolt Cs on a given chart were the same size. After verifying that the subject was ready and the NVGs were properly focussed, the experimenter initiated cart movement from the computer workstation. Upon cart movement, the subject lowered the vision occluder and viewed the acuity chart. The subject stopped the cart by depressing the trigger switch on the side stick controller when he was "virtually certain" he could determine the orientation of all of the Cs. After stopping the cart, the subject read aloud the orientation of each C. If the subject's responses were correct, the distance was recorded and the cart returned to the starting position. If an incorrect response was made or the experimenter was uncertain of the subject's response, the subject was asked to read the entire chart again. If the response was incorrect, the cart was advanced forward until the subject could correctly determine the orientation of each letter or until the end of the track was reached. After each trial, the subject raised the vision occluder and rested while the cart was returned to the starting position.

2.5 Experimental Design

This study incorporated a 2x2x4 repeated measures experimental design. The independent variables were the illumination level (0.01 and 0.25 moon), the contrast of the acuity charts (20 and 95 percent) and the signal to noise ratio (SNR) of the four image intensifying tubes (17.92, 15.28, 13.71 and 11.37). The dependent variable was visual acuity (measured as the minimum angle of resolution computed from the distance from the acuity targets when the subject correctly identified the orientation of all Cs. Each subject participated in 32 data collection trials, two at each experimental condition. The trials were grouped across the four image intensifier tubes and presented in blocks of eight. The order of presentation of the four blocks was counterbalanced across the twelve subjects.

Results

The distance from the NVG objective lens to the acuity chart was recorded on each trial and used to compute the mean resolution angle in minutes of arc for each condition. The data was then transformed to 1/min. of arc as a measure of visual acuity. For ease of interpretation, visual acuity will be used instead of resolution angle when describing the results and conclusions.

3.1 ANOVA Results

An analysis of variance (ANOVA) was conducted on the visual acuity data (1/min. of arc). The independent variables in the ANOVA were SNR of the image intensifier tube (4), illumination level (2), and contrast (2). SNR was considered a categorical independent variable in the ANOVA, since the signal-to-noise ratio may not be the only factor differentiating the four tubes tested. F tests involving effects with more than one degree of freedom in the numerator had a Geisser-Greenhouse correction performed [3]. All pairwise mean comparisons were done using paired t-tests from reduced models.

The mean visual acuity obtained for each intensifer tube as a function of contrast and illumination is in Figure 3.1. The results of the ANOVA showed significant main effects of SNR (P=0.0021), illumination (P=0.0001), and contrast (P=0.0001) on visual acuity, with increases in each variable resulting in increased visual acuity. The ANOVA revealed significant interactions for SNR by illumination (P=0.0061) and illumination by contrast (P=0.0183). A summary table of the ANOVA results is provided in Appendix A.

Tests for simple interactions were performed within the SNR by illumination interaction (displayed in Figure 3.2) to isolate the source of the interaction. The tests showed significant interaction (P=0.0131) only when tube SNR = 15.28 was used with each of the other levels of SNR, indicating that the effect of illumination was consistent across the three remaining tubes tested.

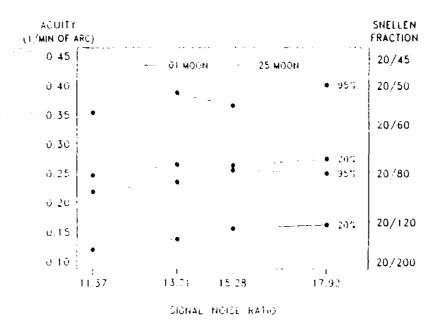


Figure 3.1: Mean visual acuity as a function of SNR, illumination, and contrast

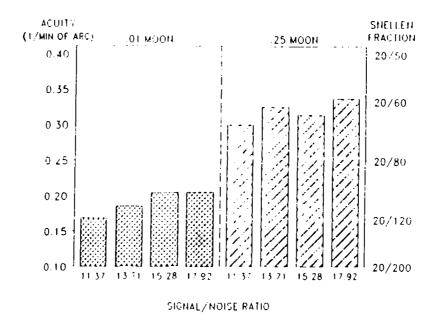


Figure 3.2: Mean visual acuity as a function of tube SNR and illumination averaged across contrast

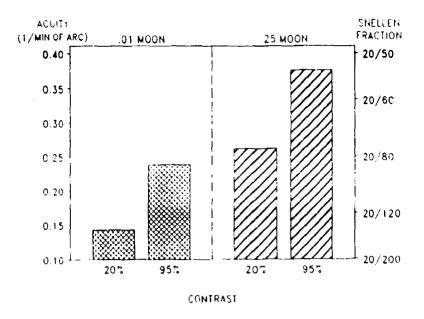


Figure 3.3: Mean visual acuity as a function of illumination and contrast averaged across SNR


Inspection of the significant illumination by contrast interaction (Figure 3.3) indicates that the mean difference in visual acuity between the two contrast conditions was significantly greater at the 0.01 moon illumination than at the 0.25 moon level. T-tests also revealed that for each level of SNR and contrast, visual acuity was significantly greater at the 0.25 moon illumination level at the 0.001 significance level.


3.2 Regression Analysis


Regression analyses were performed on the visual acuity data to obtain an estimated equation relating intensifier tube SNR to visual acuity. Separate regressions were performed for each of the four illumination and contrast conditions. In each regression, the independent variable was 1/SNR and the dependent variable was acuity in 1/min. of arc. The reciprocals were used since the relationship between SNR and acuity is asymptotic, and they provided a better fitting curve to the data than a linear model. The estimated equations are listed in Table 3.1 for each illumination and contrast condition. Plots of each estimate are displayed in Figure 3.4. Analysis of covariance indicated that the estimates describing the relationship between SNR and visual acuity did not differ significantly across the four illumination and contrast conditions, (P = 0.016).


The equations listed in Table 3.1 were used to produce tables of guidelines for predicting

percent increases in acuity for a range of SNRs from 10 to 20, (Tables 4.1 through 4.4). Relative percent increases in visual acuity predicted for the SNRs tested in this study are listed in Table 3.2 for each condition. The values in this table represent the percent increase in acuity predicted when increasing from a specific SNR value (left column) to a higher SNR value (top row). Due to the significant interaction involving tube SNR 15.28, the regression analysis was performed again without this tube included. The estimated equations for this regression are listed in Table 3.3.

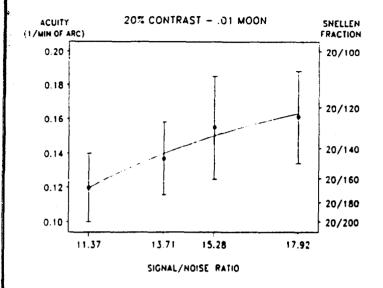

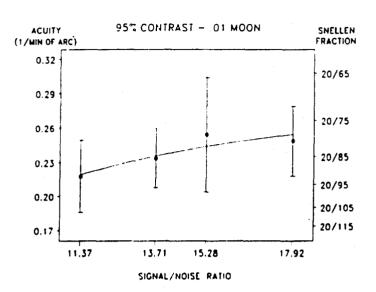

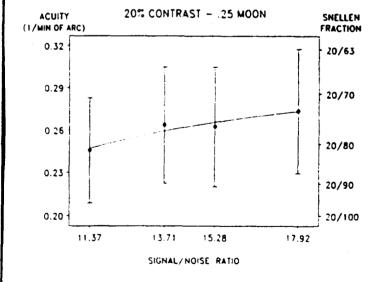

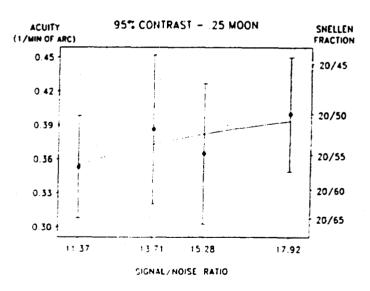

人名英格兰 有人不知道 在我的 不知道以其他以外不知,不是不知,我也是我们是我们是我们是我们的人,我不是我们是我们就是我们的人,我们们就是我们的人,我们们就是我们的人,我们们们就是我们的人,我们们们

Figure 3.4: Estimated equations depicting relationship between SNR and visual acuity for each illumination and contrast condition

Table 3.1: Estimated Equations for each illumination and contrast condition

ILLUM. LEVEL	CONTRAST	ESTIMATED EQUATION	CORR	P
0.01 MOON	20%	0.2390 - 1.3596/SNR	0.98	0.0172
0.01 MOON	95%	0.3151 - 1.0875/SNR	0.91	0.0935
0.25 MOON	20%	0.3193 - 0.8217/SNR	0.96	0.0378
0.25 MOON	95%	0.4614 - 1.2107/SNR	0.78	0.2185

Table 3.2: Percent increase in visual acuity from a lower SNR (left column) to a greater SNR (top row) between the SNRs used in this study

	i i	[SNR	
CONDITION	SNR	13.71	15.28	17.92
Illum. = 0.01	11.37	15%	20	27
Contrast = 20%	13.71	!	7	14
	15.28	l 		8
		13.71	15.28	17.92
Illum. $= 0.01$	11.37	7%	10	14
Contrast = 95%	13.71		3	7
	15.28	<u> </u>	<u> </u>	4
		13.71	15.28	17.92
Illum. $= 0.25$	11.37	5%	7	10
Contrast = 20%	13.71		2	5
	15.28	ļ	<u> </u>	3
		13.71	15.28	17.92
Illum. $= 0.25$	11.37	5%	7	10
Contrast = 95%	13.71		2	5
	15.28			3

Table 3.3: Estimated equations with tube SNR 15.28 excluded from analysis

ILLUM, LEVEL	CONTRAST	ESTIMATED EQUATION	CORR	P
0.01 MOON	20%	RES == 0.2328 - 1.2966/SNR	0.99	0.0396
0.01 MOON	95%	RES = 0.3024 - 0.9572/SNR	0.99	0.0332
0.25 MOON	20%	RES = 0.3234 - 0.8630/SNR	0.98	0.1269
0.25 MOON	95%	RES = 0.4836 - 1.4387/SNR	0.96	0.1753

Discussion

The purpose of this study was to quantify the relationship between NVG image intensifier tube signal-to-noise ratio and human visual acuity. The results showed that increases in intensifer tube SNR resulted in better visual acuity at both quarter moon and starlight illumination for both high and low contrast targets. The functions describing the relationship between SNR and acuity did not statistically differ across the four conditions tested, although there was a trend toward SNR having a greater impact on acuity under lower visibility conditions. This trend failed to reach significance due to the large amount of variability between subjects and the small number of intensifier tube SNRs tested. A study using more subjects and a greater number of SNR levels may be expected to result in a significant effect of SNR on acuity under low illumination and contrast conditions. The effects of target contrast and illumination on acuity were as expected, with higher contrast and illumination levels resulting in better visual acuity.

The results of the regression analyses were used to generate tables of guidelines for predicting percent increases in acuity as a function of SNR. These guidelines, contained in Tables 4.1 through 4.4, allow the user to estimate percent increases in visual acuity performance over an SNR range of 10 to 20. The values in the tables are estimated percent increases in visual acuity as SNR is increased from a lower value (left column) to a greater value (top row).

Inspection of these tables reveals that improvements in visual acuity with increases in SNR vary depending upon the illumination and contrast. For example, Table 4.1 shows that doubling SNR (from 10 to 20) results in a 40% improvement in visual acuity for low illumination and low contrast. However, the same increase in SNR results in only a 15% increase in acuity for both the 20% and 90% contrast targets at quarter moon illumination (Tables 4.3 and 4.4). Therefore, increases in SNR have their greatest impact on visual performance under conditions of lower illumination. This is better illustrated by the following example.

It might be expected that an individual's visual acuity performance with intensifier tubes having an SNR of 20 would be significantly better than the acuity achieved with an SNR of 15 (a 33% difference in SNR). However, the present results show that such an increase results in only an estimated 13% improvement in acuity for 20% contrast targets and a 7% improvement for the 95% contrast targets at .01 moon illumination (Tables 4.1 and 4.2). Likewise, the same increase in SNR for quarter moon illumination improves acuity by only 5% for both levels of contrast (Tables 4.3 and 4.4). This may be a negligible improvement for some NVG scenarios.

It should be noted that the values in the tables are estimated increases predicted from "best case" laboratory viewing conditions. These values also represent average increases derived from the mean acuity of the individuals tested in this study. Operational scenarios, employing other measures of acuity for different individuals, may yield different results.

Subject variability also proved to be a significant factor affecting visual acuity through NVGs in the present study. Although all subjects reported 20/20 visual acuity prior to testing, acuity for NVG viewing ranged from 20/108 to 20/175 in the most degraded visibility condition (low illumination, low contrast) and from 20/42 to 20/65 in the highest illumination and contrast condition. Inspection of the data showed only slight differences in the subjects' rank order acuity performance across the four conditions, indicating that certain subjects were consistently better in their acuity performance than others. This may have been due to differences between subjects in the criterion adopted when responding to the acuity charts. Subjects showing poorer acuity may have been more conservative in responding, causing them to come in closer to the acuity chart before making a decision; whereas, subjects with better acuity may have been less conservative in making their responses and stopped the cart at greater distances from the acuity chart. This subject variability also suggests that an individual's acuity through NVGs may not be correlated with acuity measured for unaided normal room light viewing. This could have implications for NVG selection and training criteria, where a reliable pre-flight method of determining expected acuity levels during NVG flight missions is necessary. Further research should be done to determine if a correlation exists between acuity measured for unaided viewing and NVG viewing.

Table 4.1: Prediction Matrix for SNR-Visual Acuity .01 Moon 20% Contrast

			Ī	ERO	CENT I	NCR	EAS	E IN A	CUIT	Ŷ	·			
SNR	11	11.37	12	13	13.71	14	15	15.28	16	17	17.92	18	19	20
10	11	14	18	23	26	27	31	31	33	35	37	37	38	40
11	-	3	8	14	17	19	22	23	25	27	29	29	31	33
11.37	•	-	5	11	15	16	20	20	22	25	27	27	29	30
12	-	-	-	6	10	11	15	15	17	20	22	22	24	25
13	i -	-	-	-	4	5	9	10	13	15	18	, 18	20	21
13.71	-		-	-	ļ •	1	6	7	9	12	14	14	16	18
14	i 1 -			-	-	-	4	5	8	11	13	13	15	17
15				١.		-	-	1	4	7	¦ 9	9	11	13
15.28	: : :	į -		-	·	•	-	 -	3	6	8	. 8	10	12
16	{{ }	-	-	-				i -	-	3	6	6	8	10
17	-	-	.	j .	.		.	<u> </u>		 -	3	3	5	; 7
17.92	 •	-			-	-	-		.	-	} ; -	0	3	5
18	ļ, -	-	-				; -	! ;		-	! -	! -	$\frac{1}{2}$	4
19	<u> </u>	<u> </u>	· _	<u> </u>	<u> </u>	<u> - </u>	<u> </u>		<u> </u>		! !	<u></u>	i .	: 2

Table 4.2: Prediction Matrix for SNR-Visual Acuity .01 Moon 95% Contrast

			I	PERC	CENT I	NCR	EAS	E IN A	CUIT	Ϋ́				 -
SNR	11	11.37	12	13	13.71	14	15	15.28	16	17	17.92	18	19	$\overline{20}$
10	5	6	8	11	12	13	15	15	17	18	19	$\overline{19}$	20	21
11	i - 1	1	4	7	8	9	11	11	13	14	15	15	16	17
11.37	! -	-	2	5	7	8	10	10	11	13	14	14	15	16
12	-	-	-	3	5	5	7	8	9	11	12	12	13	14
13	-	-		-	2	3	5	5	6	8	9	9	10	11
13.71		-		-	-	1	3	3	5	6	7	7	9	10
14	¦ -	-	-	•		-	2	3	4	5	7	7	8	9 !
15	j -	-	-			-		1	2	3	5	5	6	7
15.28	; -	-	-	-	; ;		-		1	3	4	4	¦ 5	6
16	-		-	-	-		i -	-	-	2	3	3	i - i	$\begin{array}{c} 1 & 5 \end{array}$
; 17	¦ -	j -	<u> </u>		, -	١.	.	i . •			1	1	! 3	i 4 j
17.92			l) -	-			-	-	!	<u> </u>	-	0	1	$\begin{array}{c c} 1 & 2 \end{array}$
18	-		-	-	-		! -	<u> </u>	<u> </u>		! : !	-	1	2
19	i . L	i -	<u> </u>	<u>. </u>		<u>.</u> 	i .	i .		, -	i . L	i .	! -	1

Table 4.3: Prediction Matrix for SNR-Visual Acuity .25 Moon 20% Contrast

			I	PERC	CENT I	NCR	EAS	E IN AC	CUIT	Ϋ́				
SNR	11	11.37	12	13	13.71	14	15	15.28	16	17	17.92	18	19	20
10	3	-4	5	7	9	9	10	11	12	12	13	13	14	15
11	-	1	2	4	6	6	8	8	9	10	11	11	11	12
11.37	-	-	2	4	5	5	7	7	8	9	10	10	11	11
12		<u>'</u>		2	3	4	5	6	6	7	j 8	8	9	10
13			-	-	1	2	3	4	4	5	6	6	7	8
13.71	i -	ļ -	ļ -	-		0	2	2	3	4	5	5	6	7
14	į .		ļ -				1	2	3	4	5	5	6	6
15	 •			¦ -	! -		١.	0	1	2	¦ 3	3	4	5
15.28	<u> </u> -	i -	-						1	2	3	3	4	5
16	-				! -	-	-	-	-	1	2	2	3	4
17	<u>.</u>	! .				-		•		-	1	1	2	3
17.92	.					-	-	-	-	-		0	1	2
18	-		-							-		i -	1	2
19	-	-	 -	-	-	-	1 -			-	<u> </u>	<u> -</u>	Ì	1

Table 4.4: Prediction Matrix for SNR-Visual Acuity .25 Moon 95% Contrast

]	ERC	CENTI	NCR	EAS	E IN A	CUIT	Ϋ́				
SNR	11	11.37	12	13	13.71	14	15	15.28	16	17	17.92	18	19	20
10	3	4	6	8	9	9	11	11	12	13	14	14	14	15
11	.	1	3	5	6	6	8	8	9	10	11	11	12	12
11.37	ļ <u>-</u>	 -	2	4	5	5	7	7	8	9	10	10	11	11
12	-	-	•	2	3	4	5	6	7	8	8	9	9	10
13	-	-			1	2	3	4	5	6	6	7	7	8
13.71	! .		.		-	0	2	2	3	4	5	5	6	7
14				-		-	2	ز إ	3	4	j 5	5	6	6
15				(} •				<u> </u>	1	2	3	3	4	5
15.28		-	-					ļ -	1	2	3	3	4	5
16	.		-	¦ .	: : -	-	-	-	-	1	2	2	3	4
17	.	.	ļ .		: -		-	-	 •	-	1	1	2	3
17.92	: -	-			-	-		.			·	0	ⁱ 1	2
18			•		.			.		-			1	2
19	; •		· •		i •			:		-	-		! .	1

Bibliography

- [1] Csorba, Illes P., IMAGE TUBES. Howard W. Sams and Co., Inc. Indianapolis, Ind. 1985.
- [2] RCA ELECTRO-OPTICS HANDBOOK. Technical Series EOH-11. RCA Corporation, 1974.
- [3] Keppel, G. DESIGN AND ANALYSIS: A RESEARCHERS HANDBOOK. Prentice Hall Inc., 1982.
- [4] Holmes, R. HUMAN FACTORS ASPECTS OF THE DESIGN OF NVGS. In Aircrew Helmets and Helmet Mounted Devices: Proceedings of the Symposium, London, England. 1987.
- [5] Field, H.P. GENERATING LOW LIGHT LEVELS FOR NIGHT VISION DEVICE EVALUATION. In Soc. of Photo-optics Instrum. Engineering Seminar Proc., Vol 33. pg. 159-163, 1972.
- [6] Levine, R.R., and Rash, C.E. VISUAL ACUITY WITH AN/PVS-5A NIGHT VI-SION GOGGLES AND SIMULATED FLASHBLINDNESS PROTECTIVE LENSES UNDER VARYING LEVELS OF BRIGHTNESS AND CONTRAST. United States Army Medical Research Laboratory (USAARL) Technical Report No. 89-16. July, 1989.
- [7] Mummaw, D.A., Ford, R.H., and Nims, D.F. AN/AVS-6 NIGHT VISION GOGGLE TEST. Air Force Flight Test Center, Edwards Air Force Base, Calif. Air Force Systems Command. AFFTC-TR-83-5. April, 1983.
- [8] Verona, R.W. IMAGE INTENSIFIERS: PAST AND PRESENT. United States Army Electronics Research and Development Command. Fort Belvoir, Va.

- [9] Wiley, R.P. VISUAL ACUITY AND STEREOPSIS WITH NIGHT VISION GOG-GLES. United States Army Medical Research Laboratory (USAARL) Technical Report No. 89-9. June, 1989.
- [10] US ARMY TEST AND EVALUATION COMMAND TEST OPERATIONS PRO-CEDURE: IMAGE INTENSIFIERS, NIGHT VISION (AN/PVS-7 GOGGLES). U.S. ARMY Report Number TOP 6-2-603, July, 1985.

Appendix

The results of the ANOVA conducted on the visual acuity data are summarized in Table 5.1 below.

Table 5.1: Analysis of Variance (ANOVA) Summary Table

SOURCE	SUM OF SQ.	NUM DF	DEN DF	F	P	P (GG.)	EPSILON
SNR	0.06769	3	33	8.55	0.0002	0.0021	0.639
ILLUM	1.57146	1	11	295.03	0.0001	NA	NΛ
CON	1.05767	1	11	423.98	0.0001	NA	NA
SNR*ILL	0.01235	3	33	6.00	0.0022	0.0061	0.7431
SNR*CON	0.00116	3	33	0.90	0.4501	0.4287	0.7481
ILL*CON	0.00890	1	11	7.66	0.0183	NA	NA
SNR*ILL*CON	0.00468	3	33	1.67	0.1926	0.2117	0.6609